

VistaPano S 2.0

The following information supplements the installation and operating instructions of the unit:




As a general rule, the installation and operating instructions of the device must also be observed. These instructions include important information such as safety instructions and information on the setup, electrical connections, disinfection process, cleaning process etc.




VATECH Co. Ltd.
13, Samsung 1-ro 2-gil
Hwaseong-si, Gyeonggi-do,
18449 Korea

Panoramic X-ray device

Inserting the positioning aids

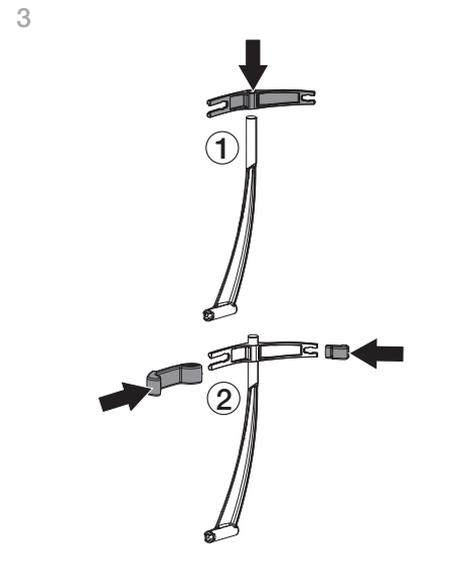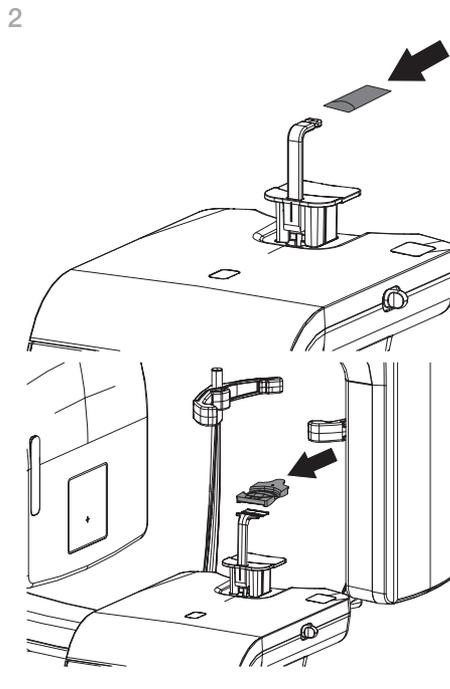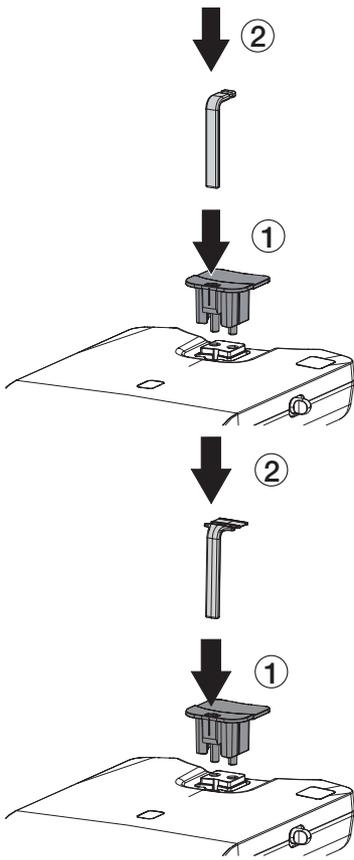


Imaging-Software setup

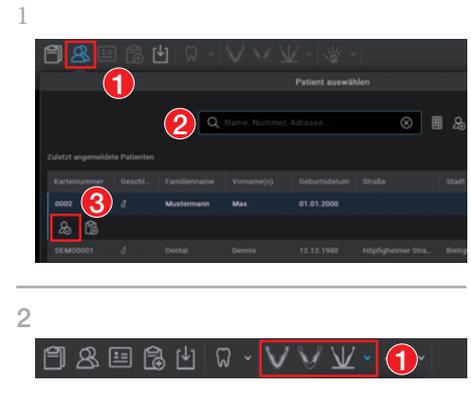


Distributed by:
Air Techniques, Inc.
1295 Walt Whitman Road
Melville, New York 11747-3062, USA

3

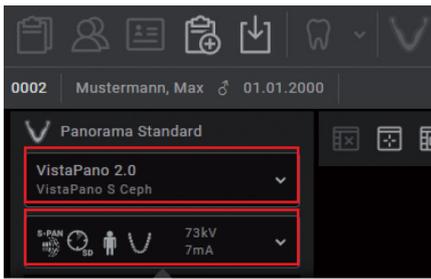


Patient positioning


1

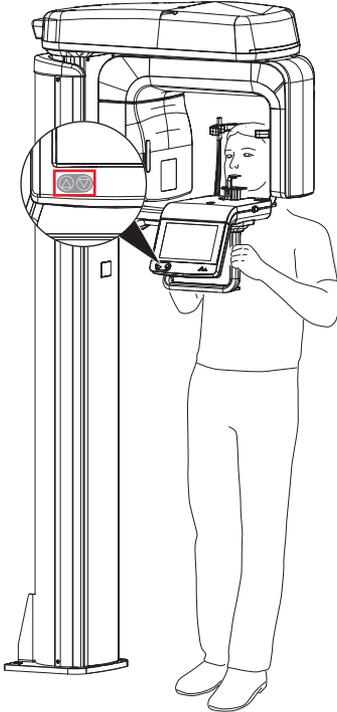


2

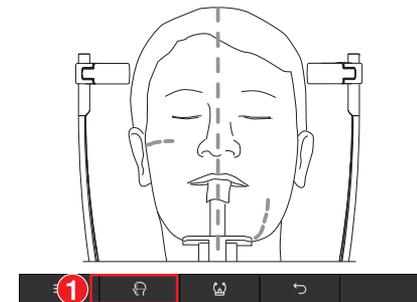

3

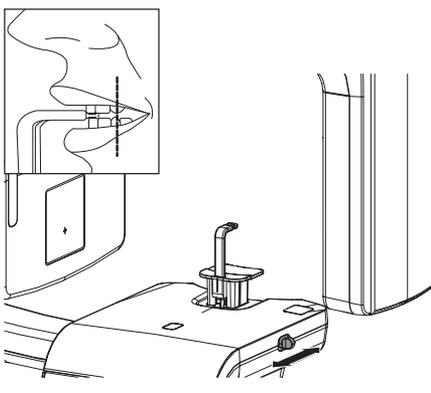


4

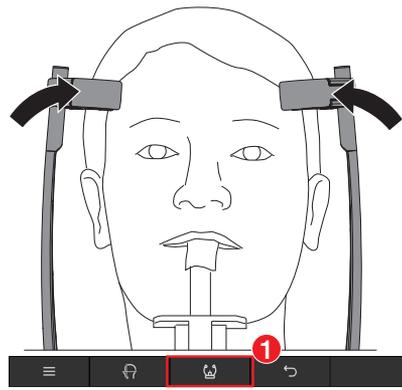

5




6

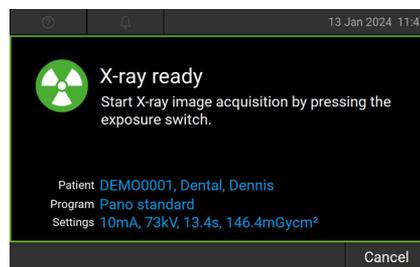


7


others

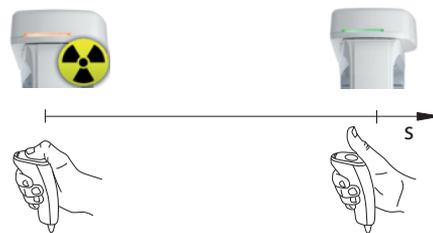

bitewing, maxillary joint

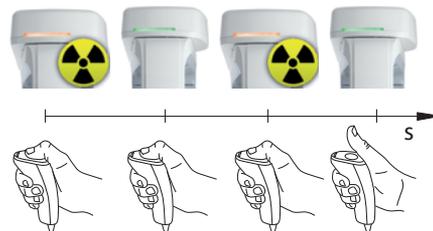


8

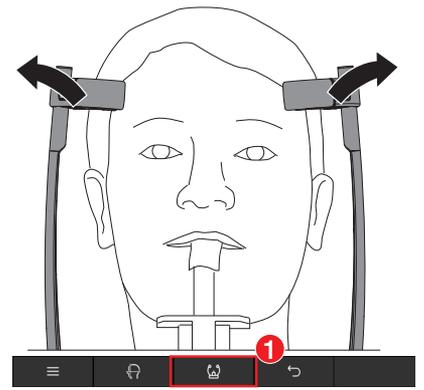


Cleaning and disinfection

1

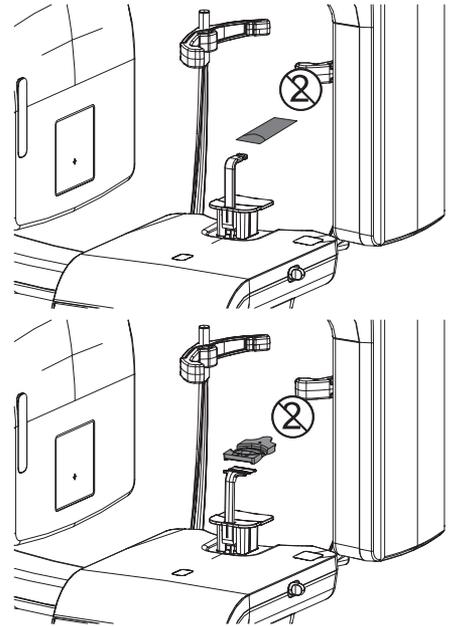

Disinfection

2





Steam sterilization

1





Ceph X-ray device






Device preparation

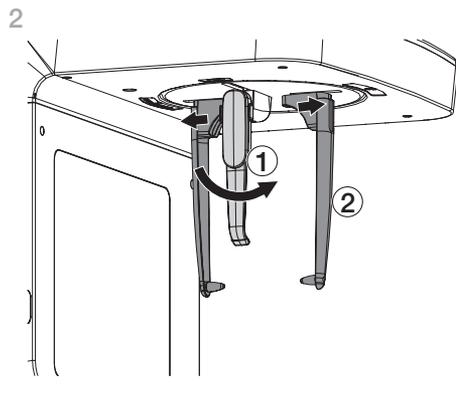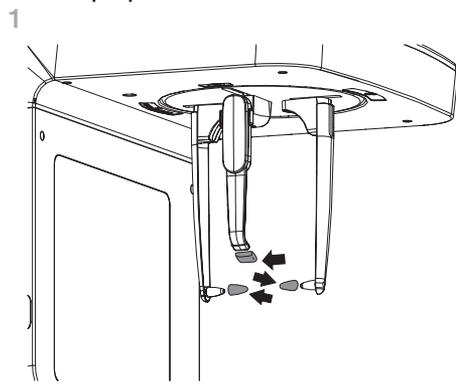


Imaging-Software setup

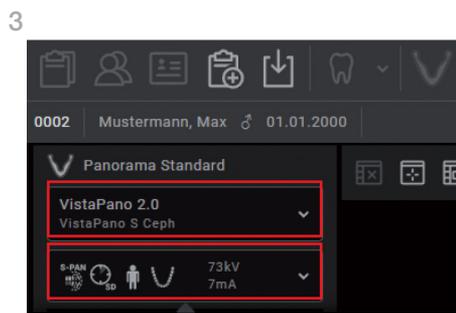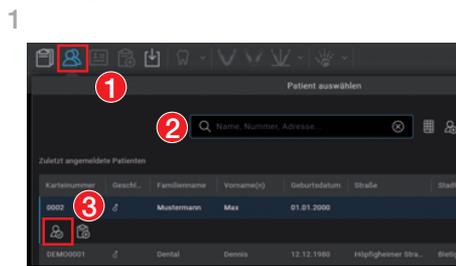


Patient positioning

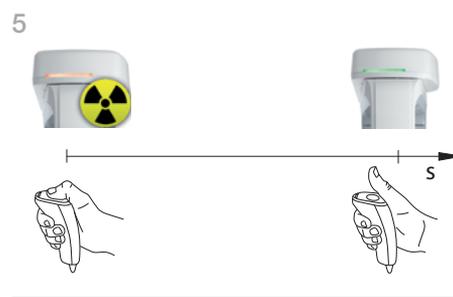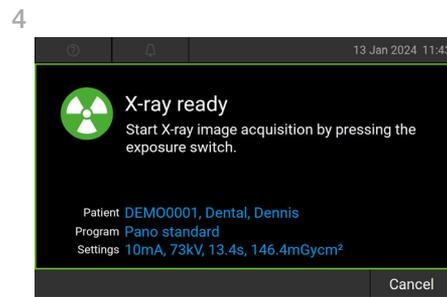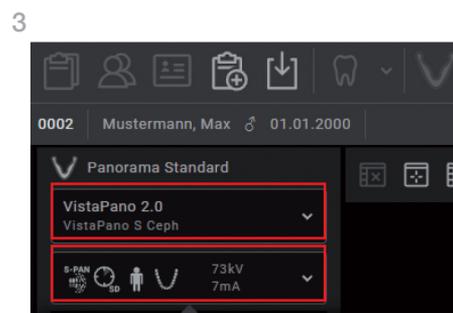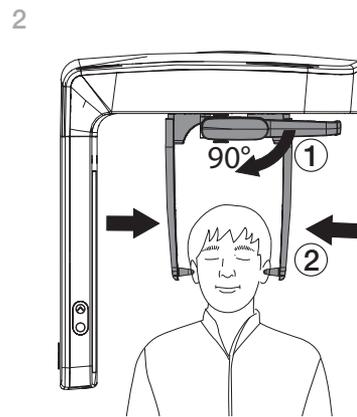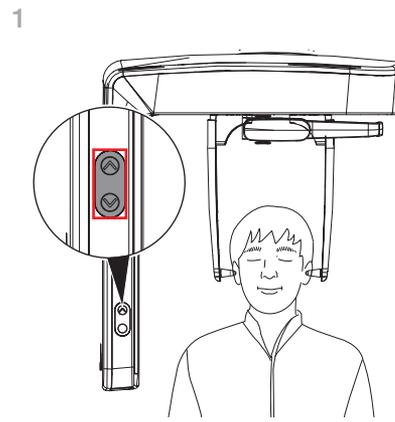

6

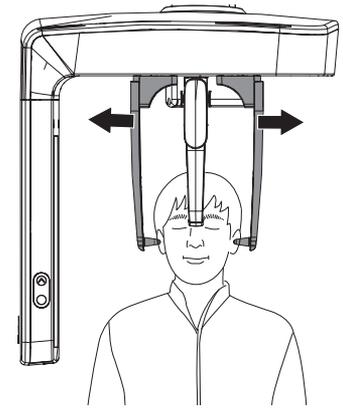

Disinfection

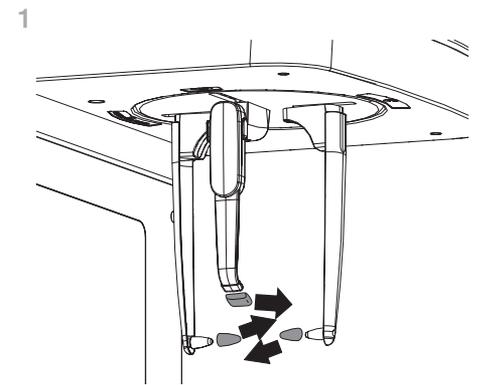

Disinfection

